



savyonDIAGNOSTICS

member of the gamida diagnostics division

savvy•gen GI- Campylobacter

REF: 606-01


Test kit for 48 determinations

Store at 2-37°C

For Professional Use Only IVD **CE**



Savyon® Diagnostics Ltd.
3 Habosem St. Ashdod 7761003
ISRAEL
Tel.: +(972).8.8562920
Fax: +(972).8.8523176
E-mail: support@savyondiagnosics.com



**European Authorized
Representative: Obelis s.a.**
Boulevard Général Wahis 53
1030 Brussels, BELGIUM
Tel: +(32) 2. 732.59.54
Fax: +(32) 2.732.60.03
E-Mail : mail@obelis.net



Intended Use

The Savvygen™GI- Campylobacter test allows the qualitative detection of Campylobacter by real time PCR in human feces. The product is intended for use in the diagnosis of Campylobacter gastrointestinal infections alongside clinical data of the patient and other laboratory tests outcomes.

For *in-vitro* professional diagnostic use.

Background

Campylobacter are gram negative, slender, spirally curved microaerophilic bacteria that live as commensal organisms in the gastrointestinal tract of many domestic and wild birds and mammals. *C. jejuni* and *C. coli* are by far the most important human pathogens in the genus and account for more than 95% of all clinical isolates worldwide.

Campylobacteriosis is the most prevalent foodborne bacterial infection in many countries including in the European Union and the United States of America. Although poultry is a major source of transmission of Campylobacter to humans, they can also be transmitted through consumption of animal products and water or via contact with animals. Another potential source of transmission is person-to-person transmission (fecal-oral or via fomites).

Campylobacteriosis is manifest as mild and self-limiting gastroenteritis characterized by vomiting and headaches followed by abdominal pain with watery or bloody diarrhea. However they have also been reported to be involved in immuno-reactivity complications and other extra gastrointestinal manifestations.

The 16S rRNA gene has been used extensively for rapid detection and identification of many bacterial taxa by Real Time PCR, including Campylobacter species.

Principles of the Procedure


The Savvygen™GI- Campylobacter test is designed for the identification of Campylobacter in human feces specimens to aid in the assessment of infections caused by these bacteria.

The Savvygen™GI- Campylobacter test is based on the real time amplification of specific conserved fragments of the 16S rRNA gene encoded by the Campylobacter genome. After DNA extraction, Campylobacter is detected by an increase in observed fluorescence during the reaction upon hydrolysis of the fluorescent probe.

The assay is based on 5' nuclease chemistry which utilizes two primers and a hydrolysis fluorogenic probe to detect the accumulation of amplified target sequence during the PCR reaction. When the polymerase begins to extend the primers, the probe is hydrolyzed by its 5' to 3' exonuclease activity causing the spatial separation of reporter and quencher. The resulting increase in fluorescence signal is proportional to the amount of amplified product in the sample and detected by the real-time PCR instrument.

The Savvygen™GI- Campylobacter test is a ready-to used test which contains in each well all the necessary reagents for real time PCR assay in a stabilized format. In addition, an internal control allows the detection of a possible reaction inhibition. The amplification of the target sequence is detected through the FAM channel whereas the internal control (IC) in HEX channel.

Materials/ Reagents Provided

Product Description	Contents
Savvygen™GI Campylobacter; 48 reactions. Cat.# 606-01 	6x Savvygen™GI- Campylobacter strips 1x Campylobacter Positive Control 1x Water RNase/DNase free 1mL 1x Rehydration Buffer 1.8 mL 1x Negative Control 1 mL Optical caps

Additional Equipment and Material Required

- Real Time PCR instrument (to check compatibility see Appendix I).
- DNA extraction kit.
- Centrifuge for 1.5 mL tubes.
- Vortex.
- Micropipettes (0.5-20 µL, 20-200 µL).
- Filter tips.
- Powder-free disposal gloves

Transport and Storage

- The reagents and the test can be shipped and stored at 2-37°C until the expiration date stated on the label.
- Positive control after resuspension should be kept at -20°C. In order to avoid repeated freeze/thaw cycles, it is recommend separating it in aliquots.
- Keep all reagents of in the dark.

Precautions

- This product is reserved exclusively for in vitro diagnostic purposes.
- Do not use after expiration date.
- Separate pre-amplification steps from post-amplification steps. Use separate locations for pre- and post-amplification. Use dedicated lab equipment for each stage. Prepare samples in a laminar flow hood using dedicated equipment to minimize contamination. Set up the post-amplification area in a low-traffic area with dedicated equipment. Follow Good Laboratory Practices. Wear protective clothing, use disposal gloves, goggles and mask.
- Use disposable containers, disposable barrier pipette tips, disposable bench pads, and disposable gloves. Avoid washable lab wear.
- Use a diluted bleach solution (0.2% sodium hypochlorite) to treat waste from the post-amplification and detection areas, as the waste contains amplicon. Use the bleach solution to wipe down equipment and bench areas, and to treat drains used to dispose of liquid waste.
- Do not eat, drink or smoke in areas when samples or test reagents are being used
- Specimens must be treated as potentially infectious as well as all reagents and materials that have been exposed to the samples and handled in the same manner as an infectious agent. Take necessary precautions during the collection, storage, treatment and disposal of samples.
- Regular decontamination of commonly used equipment is recommended, especially micropipettes and work surfaces.

Test Procedure

Specimen Collection, Processing and DNA Extraction

Stool samples should be collected in clean containers and processed as soon as possible to guarantee the quality of the test. The samples can be frozen at -20°C for longer time periods. Ensure only the amount needed is thawed because of freezing and refrosting cycles are not recommended.

For pretreatment and nucleic acid isolation, it is recommended to use your optimized manual or automatic system, and even any commercially available DNA extraction kit according to manufacturer's protocol. The assay has been validated with the following extraction kits:

- *Invisorb® Spin Universal Kit (Strattec).*
- *QIAamp DNA Stool Mini Kit (QIAGEN).*
- *QIAamp DNA Mini kit (QIAGEN).*
- *Maxwell® RSC Blood DNA Kit, using the Maxwell® 16 instrument (Promega).*
- *RIDA ® Xtract (r-Biopharm)*
- *UltraClean® Tissue & Cells DNA Isolation Kit (Mobio)*

Positive Control Preparation

Reconstitute the lyophilized *Campylobacter* Positive Control (red cap tube) with 100 µL of Water RNase/DNase free (white cap tube) supplied, vortex the tube thoroughly. After first use, dispense the Positive Control into aliquots in order to avoid multiple freeze-thaw cycles, and store at -20°C.

This component contains high copies number template and is a very significant contamination risk. Therefore, we recommend open and manipulate it in a separate laboratory area away from the other components.

PCR Protocol

Thermo-cycler program

Calculate the number of required reactions including samples and controls (At least one positive and one negative control). Set your thermos-cycler following the conditions below (Table 1):

Table 1. Real time PCR conditions

Step	Temperature	Time	Cycles
Polymerase activation	95°C	2 min	1
Denaturalization	95°C	10 sec.	45
Annealing/Extension	60°C	50 sec.	

Set the fluorescence data collection during the extension step (*) through **the FAM (*Campylobacter*) and HEX, JOE or VIC channels (Internal Control (IC))**. If you use the Applied Biosystems 7500 Fast Real-Time PCR System, the Applied Biosystems StepOne™ Real-Time PCR System or the Stratagene Mx3005P™ Real Time PCR System check that passive reference option ROX is none.

a) Reconstitute the reaction mixture of the required wells.

Calculate the number of required reactions including tested samples and controls. One positive and one negative control must be included in each run. Peel off protective aluminum seal from the strips. Pipette 15 µL of Rehydration Buffer (tube of blue cap) into each well.

b) Adding samples and controls according to real-time PCR experimental strips/plate set up.

Pipette 5 µL of Negative Control (tube of amber cap) into each negative control well. Pipette 5 µL of DNA sample into each sample well. Pipette 5 µL of reconstituted Campylobacter Positive Control (tube of red cap) into each positive control well. Cover the wells with the caps provided. Spin down briefly.

c) PCR Run.

Place the strips in the Real-Time PCR instrument and start the run.

Analysis and Interpretation of results

The analysis of the results is done by the software itself of the used real time PCR system following manufacturer's instructions.

Positive control- The positive control used in each run must show an amplification curve for Campylobacter, which validates the reaction.

Negative control- The negative control included in each run must show the absence of signal for Campylobacter, which validates the reaction.

Internal control- The Internal Controls must show amplification curves, which verify the correct functioning of the amplification mix. Sometimes, the detection of internal control is not necessary because a high copy number of the pathogen DNA template can cause preferential amplification of target sequence.

Positive sample- A sample is assigned as positive for the target if the Ct value falls below 40. The internal control usually shows an amplification signal, although it might be dispensable if the amplification of the target sequence from a high copy number of DNA template can cause competition in the reaction.

Negative sample- A sample is assigned as negative for the target if there is no evidence of amplification signal in the detection system but the internal control is positive.

Invalid run- The assay should be considered as invalid and a new run should be performed if there is signal of amplification in negative control or absence of signal in the positive well.

Note: *If a negative sample do not show an amplification curve for the internal control, they should be retested by dilution of the original sample 1:10 or the nucleic acid extraction has to be repeated due to possible problems caused by PCR inhibitors*

The result interpretation is summarized in the following table:

Table 2. Results interpretation

Campylobacter	Internal control	Negative control	Positive control	Interpretation
Positive	Positive/Negative	Negative	Positive	<i>Campylobacter</i> Positive
Negative	Positive	Negative	Positive	<i>Campylobacter</i> Negative
Positive	Positive	Positive	Positive	Experiment fail
Negative	Negative	Negative	Negative	Experiment fail

Positive: Amplification signal; **Negative:** No amplification signal

Limitations of the test

- This test provides a presumptive diagnosis of *Campylobacter* infection. All results must be interpreted together with other clinical information and laboratory findings available to the physician.
- This assay should be used only with samples from human feces. The use of other samples has not been established.
- The quality of the test depends on the quality of the sample; proper DNA from fecal specimens must be extracted. Unsuitable collection, storage and/or transport of specimens may give false negative results.
- Extremely low levels of target below the limit of detection may be detected, but results may not be reproducible.
- There is a possibility of false positive results due to cross-contamination by *Campylobacter*, either samples containing high concentrations of target DNA or contamination due to PCR products from previous reactions.

Quality Control

In order to confirm the appropriate performance of the molecular diagnostic technique, an Internal Control (IC) is included in each reaction. Besides, a positive and a negative control must be included in each assay to interpret the results correctly.


Performance Characteristics

Clinical sensitivity and specificity

Overall, 104 faecal samples from symptomatic patients were tested by Real Time PCR using: i) Savvygen™GI- *Campylobacter* test; and ii) RIDA®GENE Bacterial Stool Panel II (R-Biopharm). *Campylobacter* were detected in 42 samples by Savvygen™GI- *Campylobacter* test. This test identified even three additional positives that could be confirmed by evaluation with an additional commercial Real

Time PCR Kit (Mericon-Campylobacter spp. Kit (QIAGEN). The results show a high sensitivity and specificity to detect Campylobacter using Savvygen™ GI- Campylobacter test.

Analytical sensitivity

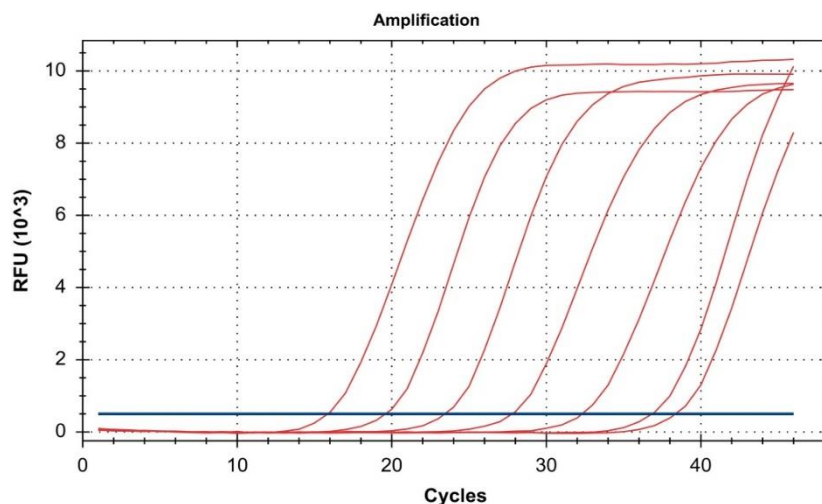

This assay has a detection limit of ≥ 10 DNA copies per reaction (Figure 1).

Figure 1. Amplification plot for 10-fold dilution series of Campylobacter template ranging from 10^7 to 10^1 copies/reaction.

Analytical specificity


The analytical specificity for Campylobacter was tested within the panel of following microorganisms, where no cross-reactivity was seen between any of the species.

Table 3. Cross-reactivity testing.

Adenovirus 40/41	<i>Enterococcus faecalis</i>	<i>Salmonella paratyphi A</i>
Astrovirus Genotype I-VIII	<i>Enterotoxigenic E. coli (ETEC)</i>	<i>Salmonella paratyphi B</i>
Norovirus GI and GII	<i>Enteropathogenic E. coli (EPEC)</i>	<i>Salmonella typhimurium</i>
Rotavirus A	<i>Giardia intestinalis</i>	<i>Salmonella bongori</i>
<i>Aeromonas hydrophila</i>	<i>Helicobacter pylori</i>	<i>Salmonella enteritidis</i>
<i>Arcobacter butzleri</i>	<i>Helicobacter hepaticus</i>	<i>Salmonella enterica</i>
<i>Bacteroides fragilis</i>	<i>Helicobacter cinaedi</i>	<i>Salmonella pullorum</i>
<i>Candida albicans</i>	<i>Helicobacter heilmannii</i>	<i>Salmonella gallinarum</i>
<i>Citrobacter freundii</i>	<i>Klebsiella oxytoca</i>	<i>Serratia liquefaciens</i>
<i>Clostridium difficile</i>	<i>Listeria monocytogenes</i>	<i>Shigella flexneri</i>
<i>Clostridium perfringens</i>	<i>Pseudomonas aeruginosa</i>	<i>Shigella dysenteriae</i>
<i>Cryptosporidium parvum</i>	<i>Proteus vulgaris</i>	<i>Staphylococcus aureus</i>
<i>Entamoeba histolytica</i>	<i>Salmonella typhi</i>	<i>Vibrio parahaemolyticus</i>
		<i>Y. enterocolitica</i> O:3 / O:9

Analytical reactivity

The reactivity of Savvygen™ GI- Campylobacter test was confirmed by the real time amplification using *Campylobacter jejuni* subsp. *jejuni*, *Campylobacter coli*, *Campylobacter lari*, *Campylobacter upsaliensis*, *Campylobacter fetus*, *Campylobacter concisus*, *Campylobacter hyointestinalis*, *Campylobacter gracilis*, *Campylobacter helveticus*, *Campylobacter curvus* and *Campylobacter rectus* as template.

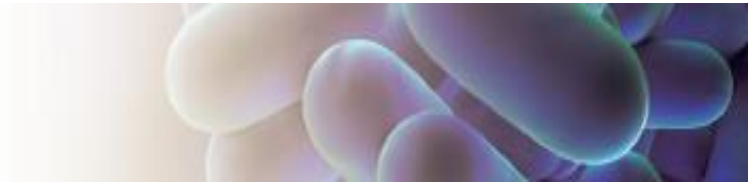

Appendix A: Compatibility of the Savvygen GI Assays with Commercial Real-Time instruments

Savvygen™ GI- Campylobacter assay has been validated on the following equipments: Applied Biosystems 7500 Fast Real-Time PCR System, Applied Biosystems StepOne™ Real-Time PCR System, Bio-Rad CFX96 Touch™ Real-Time PCR Detection System, AriaMx Real-Time PCR System, DNA-Technology DTPrime Real Time Detection Thermal Cycler. When using the Applied Biosystems 7500 Fast with strips it is recommend to place a plate holder to reduce the risk of crushed tube (Ref. PN 4388506). Additional compatible thermocyclers are listed below:

Applied Biosystems

- 7500 Fast Real-Time PCR System
- 7500 Fast Dx Real-Time PCR System
- QuantStudio™ 12K Flex 96-well Fast
- QuantStudio™ 6 Flex 96-well Fast
- QuantStudio™ 7 Flex 96-well Fast
- QuantStudio™ 3 Real-Time PCR System
- QuantStudio™ 5 Real-Time PCR System
- StepOne Plus™ Real-Time PCR System
- StepOne™ Real-Time PCR System
- ViiA™ 7 Fast Real-Time PCR System

Bio-Rad

- CFX96 Touch™ Real-Time PCR Detection System
- Mini Opticon™ Real-Time PCR Detection System

Roche

- LightCycler ®480 Real-Time PCR System
- LightCycler ®96 Real-Time PCR System

Agilent Technologies

- AriaMx Real-Time PCR System











DNA-Technology

- DTlite Real-Time PCR System
- DT prime Real-Time Detection Thermal Cycler

Bibliography

1. Bolton DJ. *Campylobacter* virulence and survival factors. *Food Microbiol* 2015; 48: 99-108.
2. Josefsen MH, Bhunia AK, Engvall EO, Fachmann MS, Hoorfar J. Monitoring *Campylobacter* in the poultry production chain – from culture to genes and beyond. *J Microbiol Methods* 2015; 112: 118-125.
3. Lund M, Nordentoft S, Pedersen K, Madsen M. Detection of *Campylobacter* spp. in chicken fecal samples by real-time PCR. *J Clin Microbiol* 2004; 42(11): 5125-5132.
4. Botteldoorn N1, Van Coillie E, Piessens V, Rasschaert G, Debruyne L, Heyndrickx M, Herman L, Messens W. Quantification of *Campylobacter* spp. in chicken carcass rinse by real-time PCR. *J Appl Microbiol* 2008; 105(6): 1909-1918.

Symbols for IVD Components and Reagents

 IVD	For <i>in vitro</i> diagnostic use only	 Keep dry	 Use by	 Manufacturer	 LOT	Lot number	
 Consult instructions for use		 Temperature limitation	 Contains sufficient for <n> test	DIL	 Buffer (sample diluent)	 REF	Catalogue number

CFX™ and IQ5™ are registered trademarks of Bio-Rad Laboratories

ABI®, QuantStudio™, StepOnePlus™ and ViiA™ are registered trademarks of Thermo Fisher Scientific Inc.

LightCycler® is a registered trademark of Roche

Mx3000P™ and Mx3005™ are registered trademarks of Agilent Technologies

Mastercycler™ is a registered trademark of Eppendorf.

Rotor-Gene® Q is a registered trademark of Qiagen.

SmartCycler® is a registered trademark of Cepheid.